




REPLACEMENT SHEET

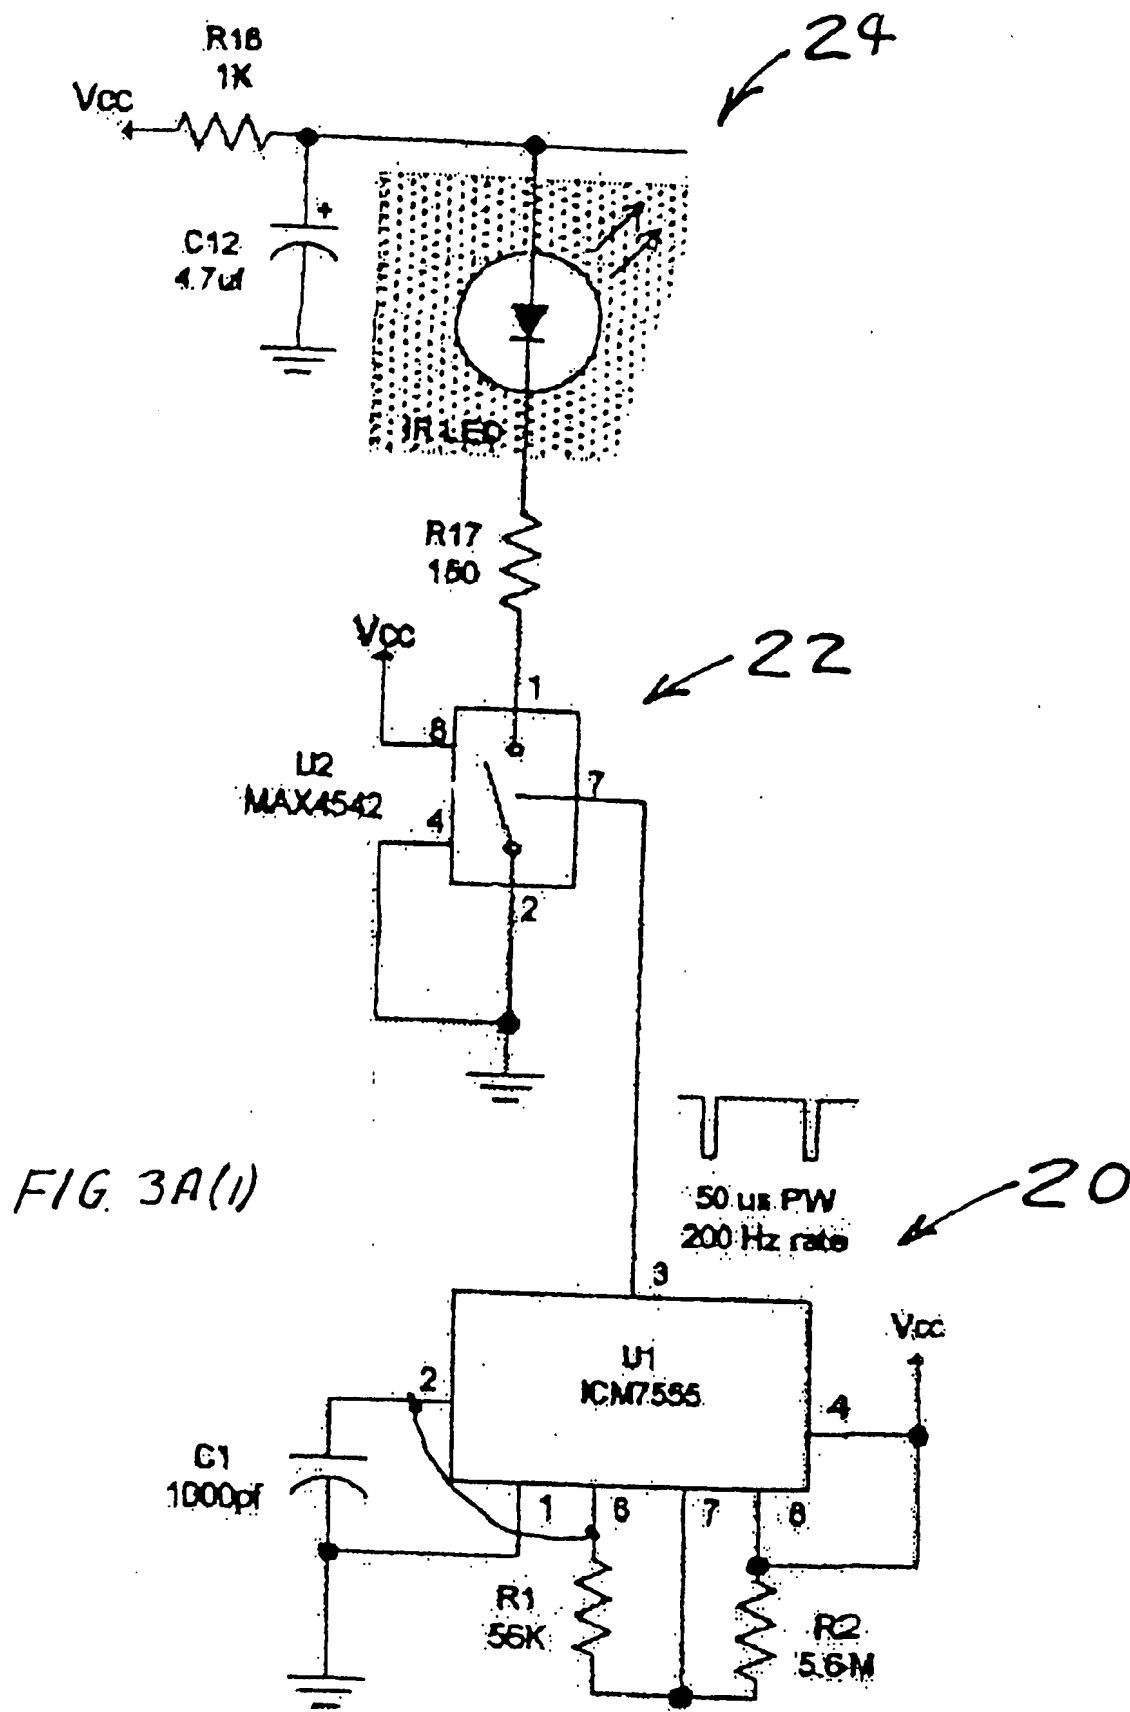

REPLACEMENT SHEET

FIG. 3A(2)

REFLECTIVE SENSOR

EE-SY-124




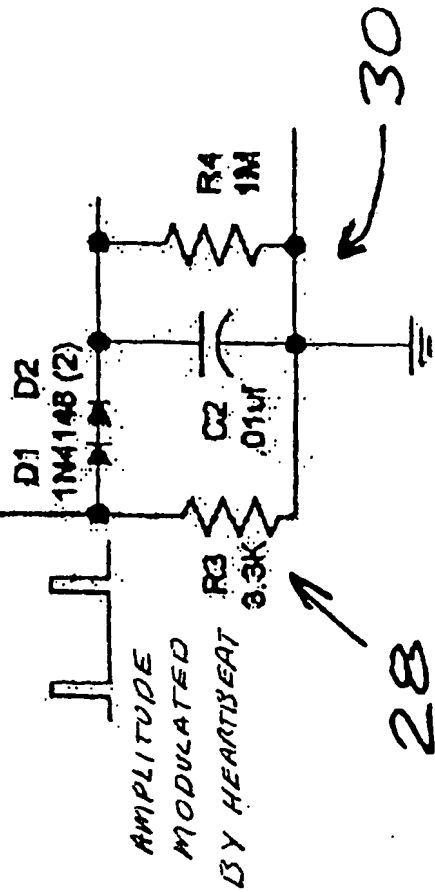


FIG. 3A(3) V_{CC}

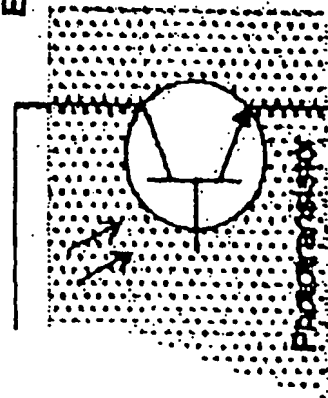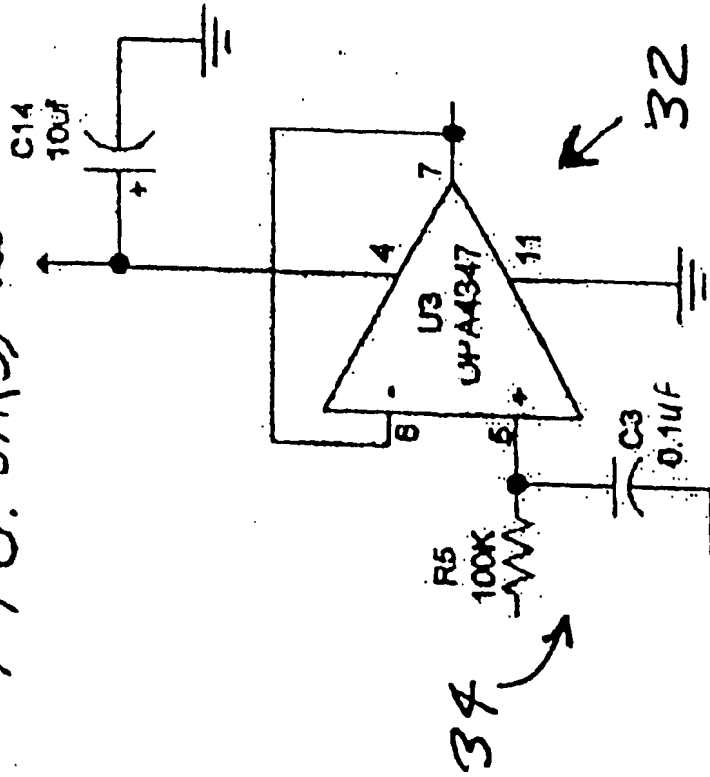

REPLACEMENT SHEET

FIG. 3A(4)

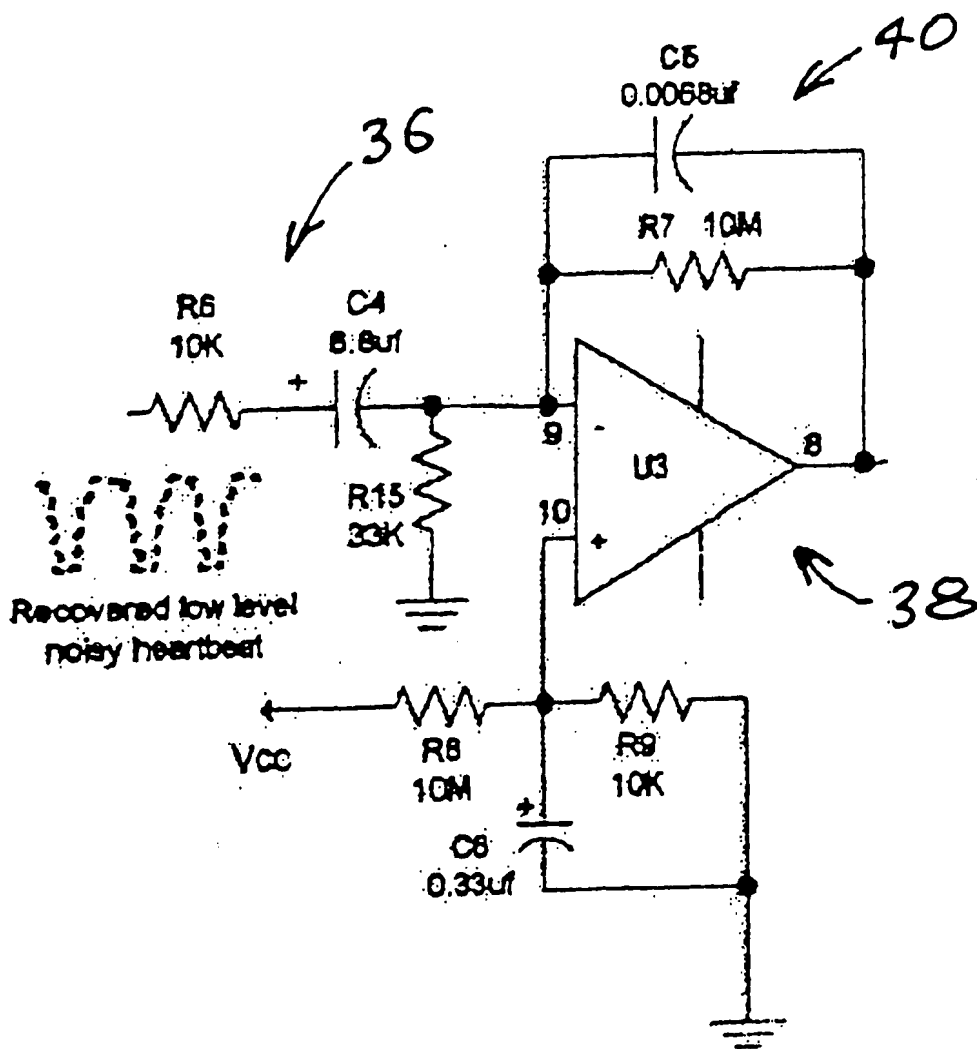

REPLACEMENT SHEET

FIG. 3A(5)

Amplified and
filtered heartbeat



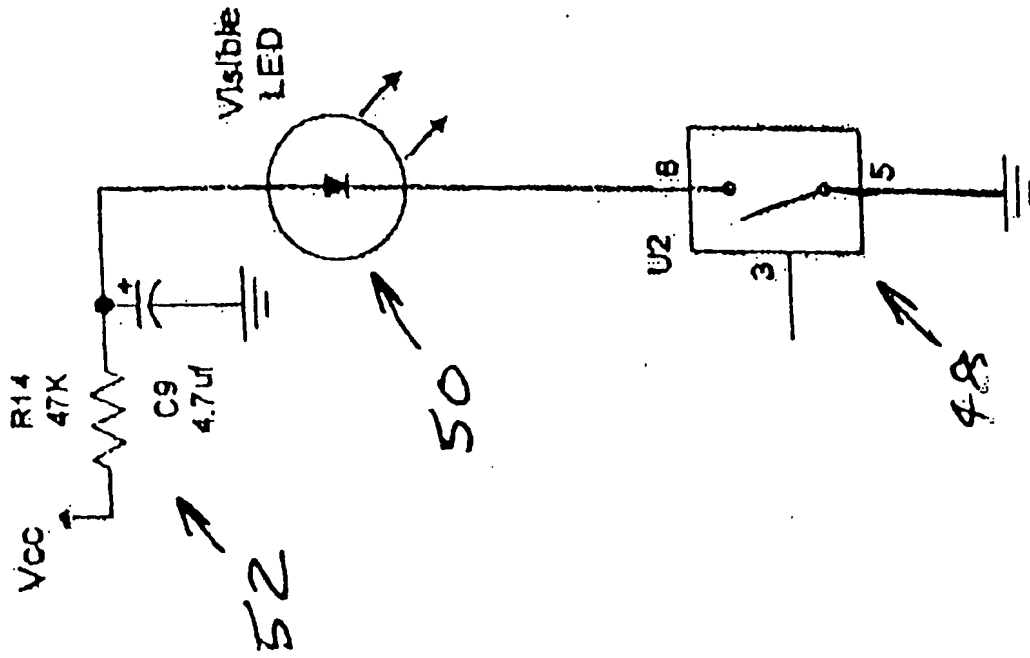


FIG. 3A(6)

REPLACEMENT SHEET

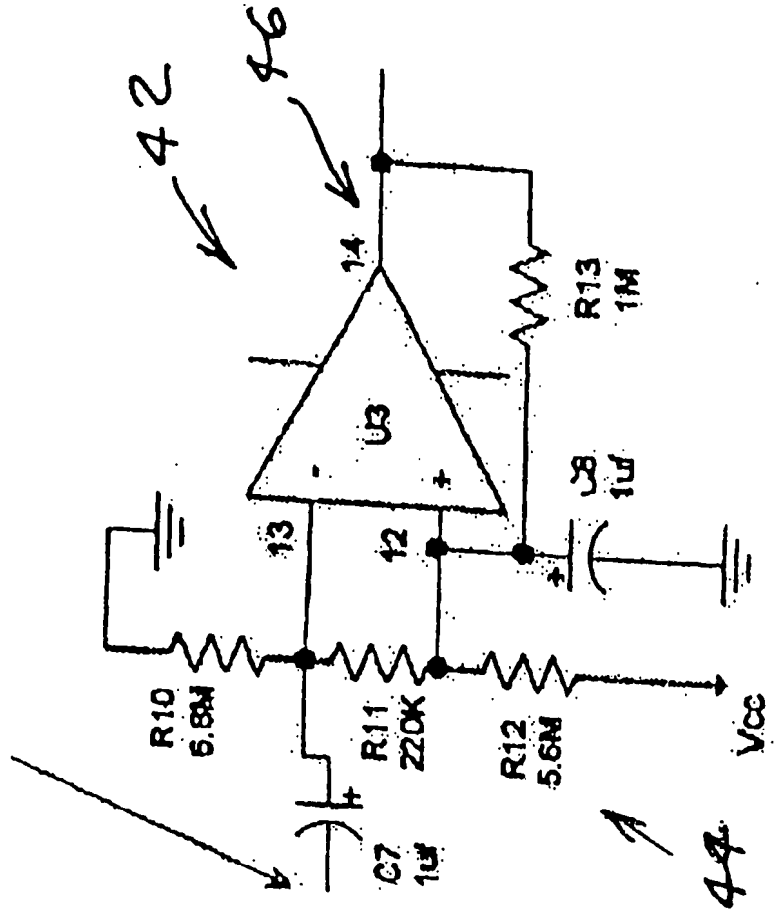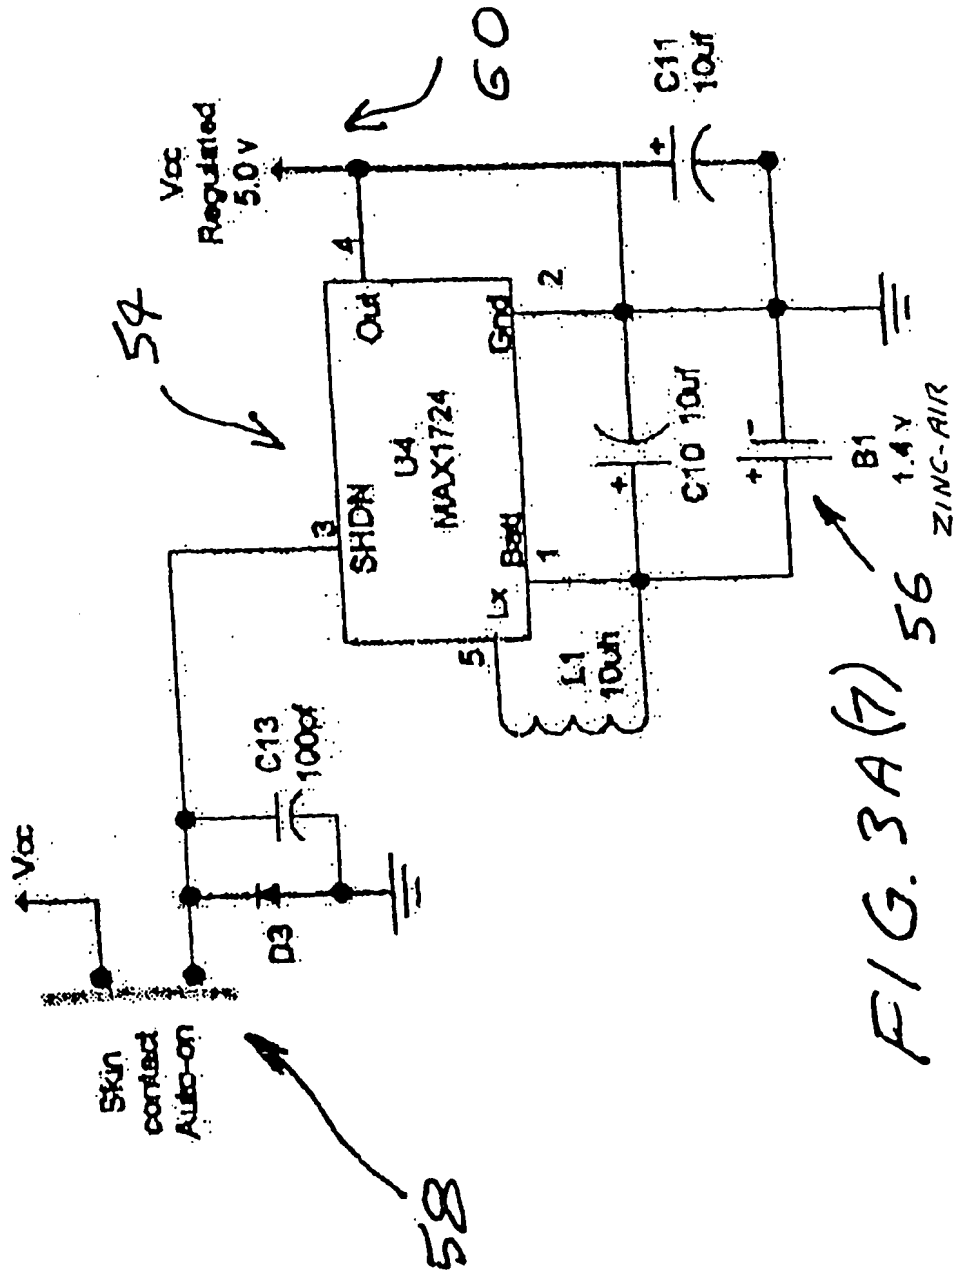

REPLACEMENT SHEET

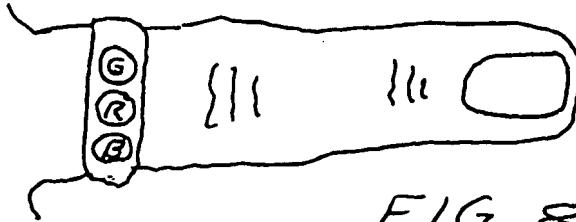


FIG. 8

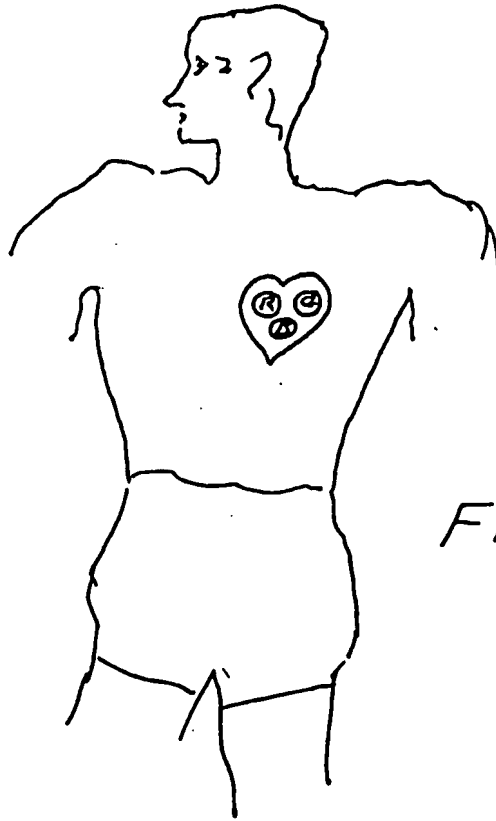


FIG. 9